

HPLC Report

Sample name: XLJT

Sequence:

Mobile phase: A: 0.1% TFA in H2O


B: 0.1% TFA in ACN

Gradient: 21-4 1%B in 20min Flow rate: 1.0ml/min

Column: Welch, C18, 4.6*150mm, 5um

Inject Date: 06/06/2018

Inj.Vol: 10uL

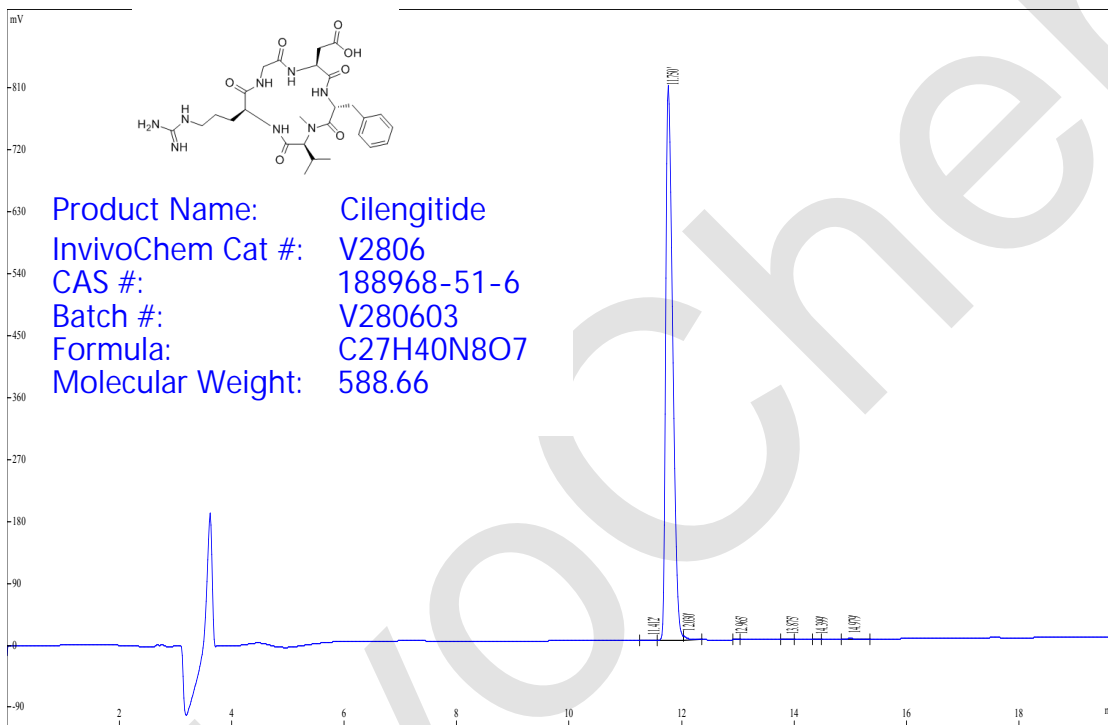

Area Percent Report

VWD: 220nm

Results

Pk#	Retention Time	Area Percent(%)	Area
1	11.412	0.1001	7010
2	11.750	99.37	6956970
3	12.030	0.353	24716
4	12.965	0.007068	495
5	13.875	0.02582	1808
6	14.399	0.0197	1379
7	14.979	0.1256	8796
Total		100	7001174