



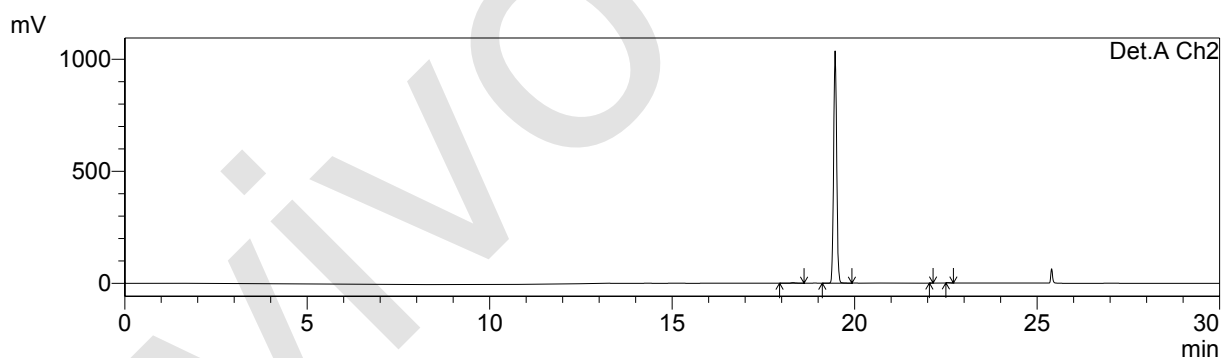

## HPLC Report

Column : Diamonsil C18(2), 5um 4.6\*250mm  
 Mobile phase : Solvent A: H2O(0.05%H3PO4) Solvent B:ACN(0.05%H3PO4)  
 Temperature : 35 °C  
 Flow rate : 0.8mL/min  
 Run time : 6min gradient(5%B), 9min gradient (5%-95%B), 5min gradient (95%B),then 5min @(5%B)  
 Detector : UV  
 Wavelength : 220/254 nm  
 User name : 846557-71-9  
 Sample name : 846557-71-9

Data File Name : 846557-71-9.lcd  
 Method File Name : 846557-71-9.lcm  
 Batch File Name : 20180421.lcb  
 Data Acquired : 2018-4-21 11:24:17  
 Data Processed : 2018-4-21 12:03:05

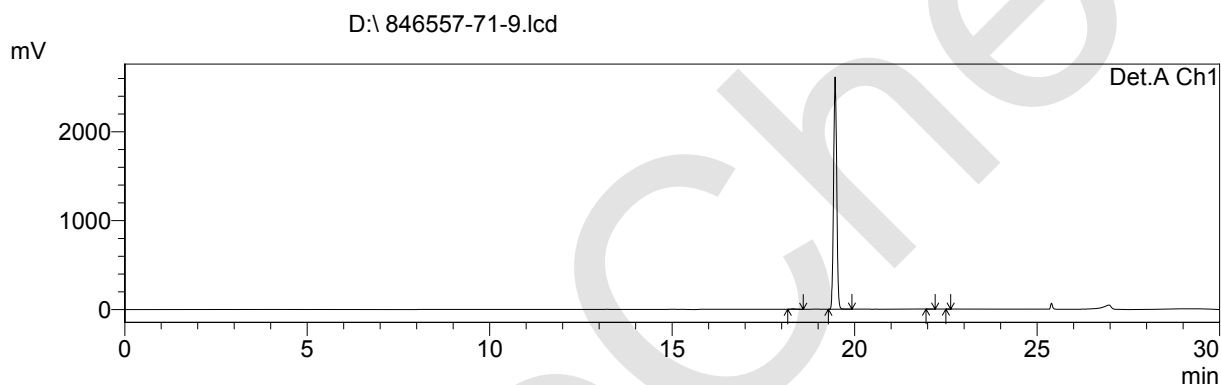

1Det.A Ch1/220nm  
 2Det.A Ch2/254nm

PeakTable

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Area %	Theoretical Plate#
1	18.307	45874	0.292	142424.873
2	19.462	15627597	99.587	207897.898
3	22.088	14736	0.094	253539.033
4	22.553	4243	0.027	477396.679
Total		15692450	100.000	



## PeakTable

Detector A Ch2 254nm

Peak#	Ret. Time	Area	Area %	Theoretical Plate#
1	18.307	19134	0.313	145816.717
2	19.461	6091452	99.562	213687.323
3	22.090	913	0.015	747717.458
4	22.553	6753	0.110	393457.646
Total		6118253	100.000	

\*\*\* End Of Report \*\*\*