


# <sup>1</sup>H-NMR Analysis for AUNP-12



MS Spectrum

Positive

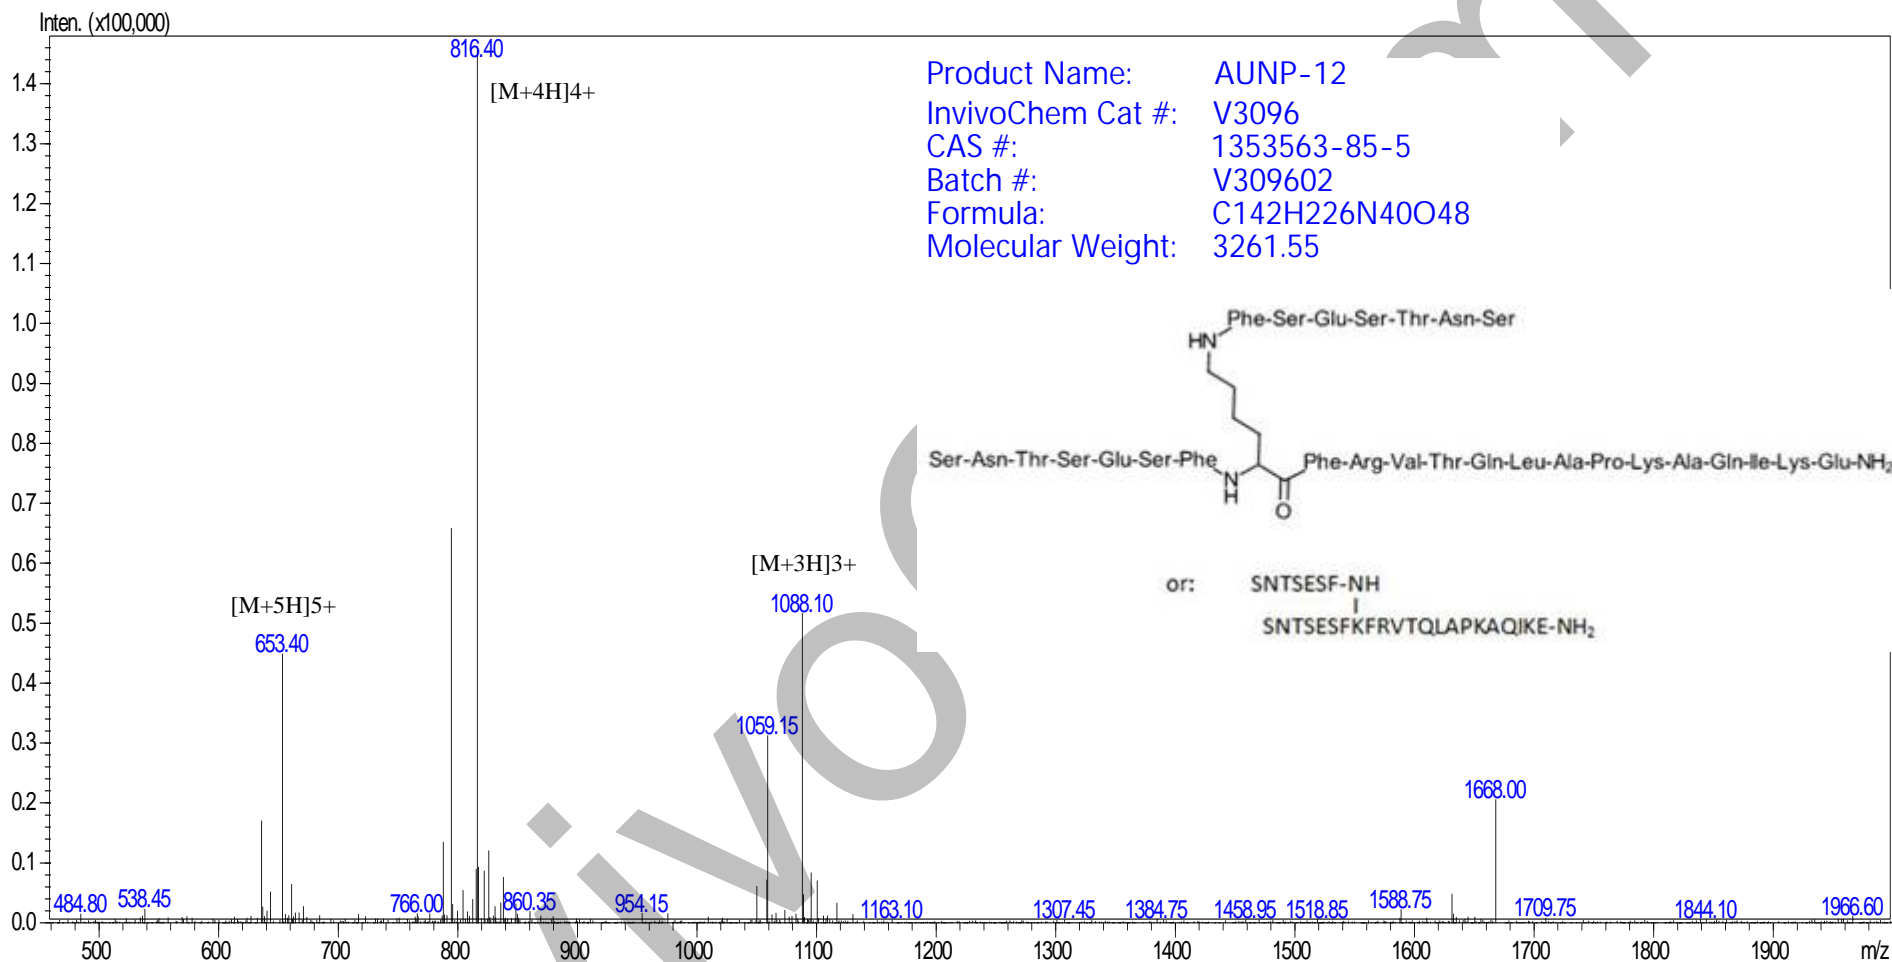

Acquired by :Shen  
Data Acquired : 2019/10/10  
Injection Volume : 1  
Sample Name : AUNP-12 SE-22  
Mw : 3261.62  
Lot No. : P190318-2-CQ715244

Probe :ESI  
Nebulizer Gas Flow :1.5L/min  
CDL :-20.0v  
CDL Temp :250°C  
Block Temp :400°C  
Probe bias :+4.5kv  
Detector :1.2kv  
T.Flow :0.2ml/min  
B.conc :50%H<sub>2</sub>O/50%ACN